


Normal Human CD3+ Pan T Cells

HC-0026

HC-0027



This product is for Research Use Only.
This product is not approved for human or
veterinary use or for use in in vitro
diagnostics or clinical procedures.

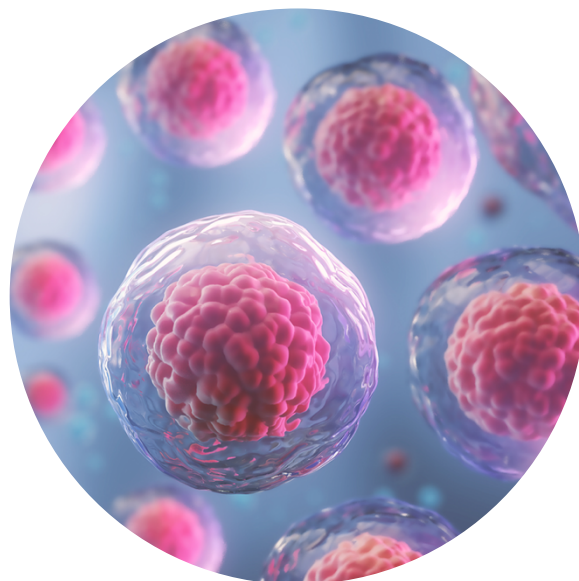


LIFELINE[®]
CELL TECHNOLOGY

Better Solutions for
Breakthrough Results

Product Description

Lifeline's Human CD3+ Pan T Cells provide an ideal culture model for the study of immunology, immunotherapy, autoimmunity, cancer, cell-based therapies, and infectious diseases. Lifeline's Human CD3+ Pan T Cells are purified from leukapheresed peripheral blood using immunomagnetic negative selection.

Human CD3+ Pan T Cells are cryopreserved directly after isolation to ensure optimal phenotype and the highest viability. Our Human CD3+ Pan T Cells are quality tested via flow cytometry to ensure proper expression of multiple markers of various hematopoietic lineage cells.

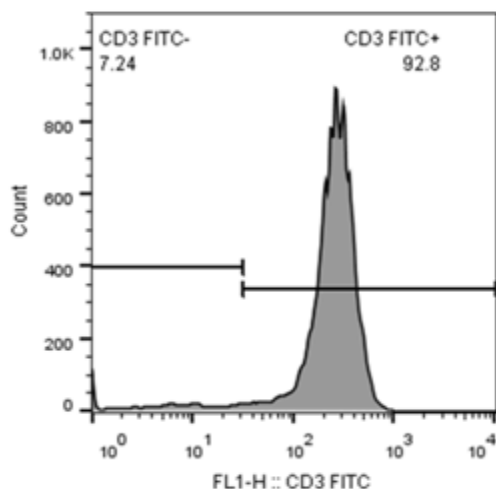


T Cells after purification

Lifeline's CD3+ Pan T Cells are

maintained in a suspension culture. CD3+ Pan T cells will not proliferate under maintenance conditions. Please refer to the respective instruction sheets for further details.

Lifeline's CD3+ Pan T Cells have not been exposed to antimicrobials or phenol red. Although antimicrobials are not required for eukaryotic cell proliferation, they are recommended to inhibit potential fungal or bacterial contamination of eukaryotic cell cultures. A vial of Gentamicin and Amphotericin B (GA [LS-1117](#)) is provided with the purchase of RPMI-1640 Medium Complete Kit ([LL-0066](#)) for your convenience.

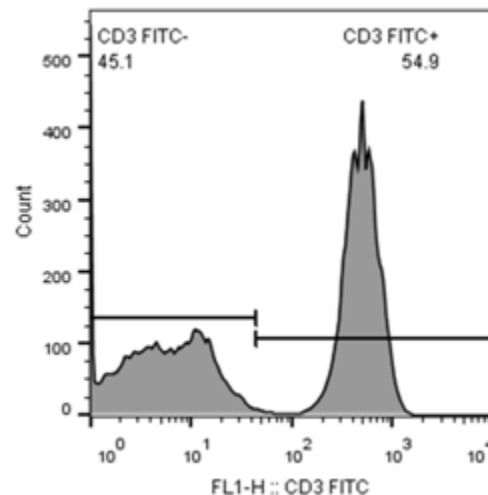

T Cells before purification

CELL FEATURES:

- Human CD3+ Pan T Cells are cryopreserved at 5×10^6 or 10×10^6 cells per vial.
- Human CD3+ Pan T Cells are extensively tested for quality and optimal performance.
- Lifeline guarantees performance and quality.



Call Lifeline Technical Service and Sales at **877.845.7787**

Or visit lifelinecelltech.com for more information

Lifeline Cell Technology | 8415 Progress Drive, Suite T | Frederick, MD 21701

©2024 Lifeline Cell Technology, an International Stem Cell Company | All Rights Reserved

HUMAN CD3+ PAN T CELLS ARE TESTED FOR:

• Cell Count	Human CD3+ Pan T Cells $\geq 5 \times 10^6$ cells per vial Human CD3+ Pan T Cells $\geq 10 \times 10^6$ cells per vial
• Cell Viability	Minimum 80% viability when thawed from cryopreservation
• Sterility Testing	Negative for mycoplasma Negative for bacterial and fungal growth
• Virus Testing	Negative for HIV-1, HIV-2, HBV, and HCV by PCR
• Flow Cytometry Analysis	Tested for CD3, CD4, CD8 > 80% positive for CD3

Part #	Description
HC-0026	Human CD3+ Pan T Cells - 5×10^6 cells per vial
HC-0027	Human CD3+ Pan T Cells - 10×10^6 cells per vial
LL-0066	RPMI 1640 Medium Complete Kit (RPMI 1640 Basal Medium, Fetal Bovine Serum, Gentamicin and Amphotericin B)
LM-0025	RPMI 1640 Basal Medium, 100 ml
LS-1012	Fetal Bovine Serum, LS-1012, 10 ml
LS-1117	GA Antimicrobial Supplement, 1.0 mL (Gentamicin 3.0 mg/mL, Amphotericin B 1.5 μ g/mL)
LL-0076	CD3+ Pan T Cells, 5M System Complete Kit (includes LL-0066 + HC-0026)
LL-0077	CD3+ Pan T Cells, 10M System Complete Kit (includes LL-0066 + HC-0027)

Quality Tested for Guaranteed Consistency and Reproducible Results

Lifeline Cell Technology manufactures products using the highest quality raw materials and incorporates extensive quality assurance in every production run. Exacting standards and production procedures ensure consistent performance.

The Lifeline Guarantee

Lifeline's rigorous quality control ensures sterility and performance to standardized testing criteria. Upon request, Lifeline will provide lot specific QC test results, material safety data sheets, and certificates of analysis. See complete guarantee/warranty statement at lifelinecelltech.com or contact your Lifeline representative for more information.

All donated tissues have been obtained under proper informed consent and adheres to the Declaration of Helsinki, CFR Title 21 part 1271, and HIPAA Regulations relative to obtaining and handling human tissue for Research Use.



Call Lifeline Technical Service and Sales at **877.845.7787**

Or visit lifelinecelltech.com for more information

Lifeline Cell Technology | 8415 Progress Drive, Suite T | Frederick, MD 21701

©2024 Lifeline Cell Technology, an International Stem Cell Company | All Rights Reserved

Safety Statement

Lifeline recommends storing cryopreserved vials in liquid nitrogen vapor phase. Handle cryopreserved vials with caution. Always wear eye protection and gloves when working with cell cultures. Aseptically vent any liquid nitrogen from cryopreserved vials by carefully loosening the vial cap in a biosafety cabinet prior to thawing the vials in a water bath. If vials must be stored in liquid phase, the vials should be transferred to vapor phase storage or -80°C for up to 24 hours prior to being thawed.



Call Lifeline Technical Service and Sales at **877.845.7787**

Or visit **lifelinecelltech.com** for more information

Lifeline Cell Technology | 8415 Progress Drive, Suite T | Frederick, MD 21701

©2024 Lifeline Cell Technology, an International Stem Cell Company | All Rights Reserved